


OPER

TOOLS

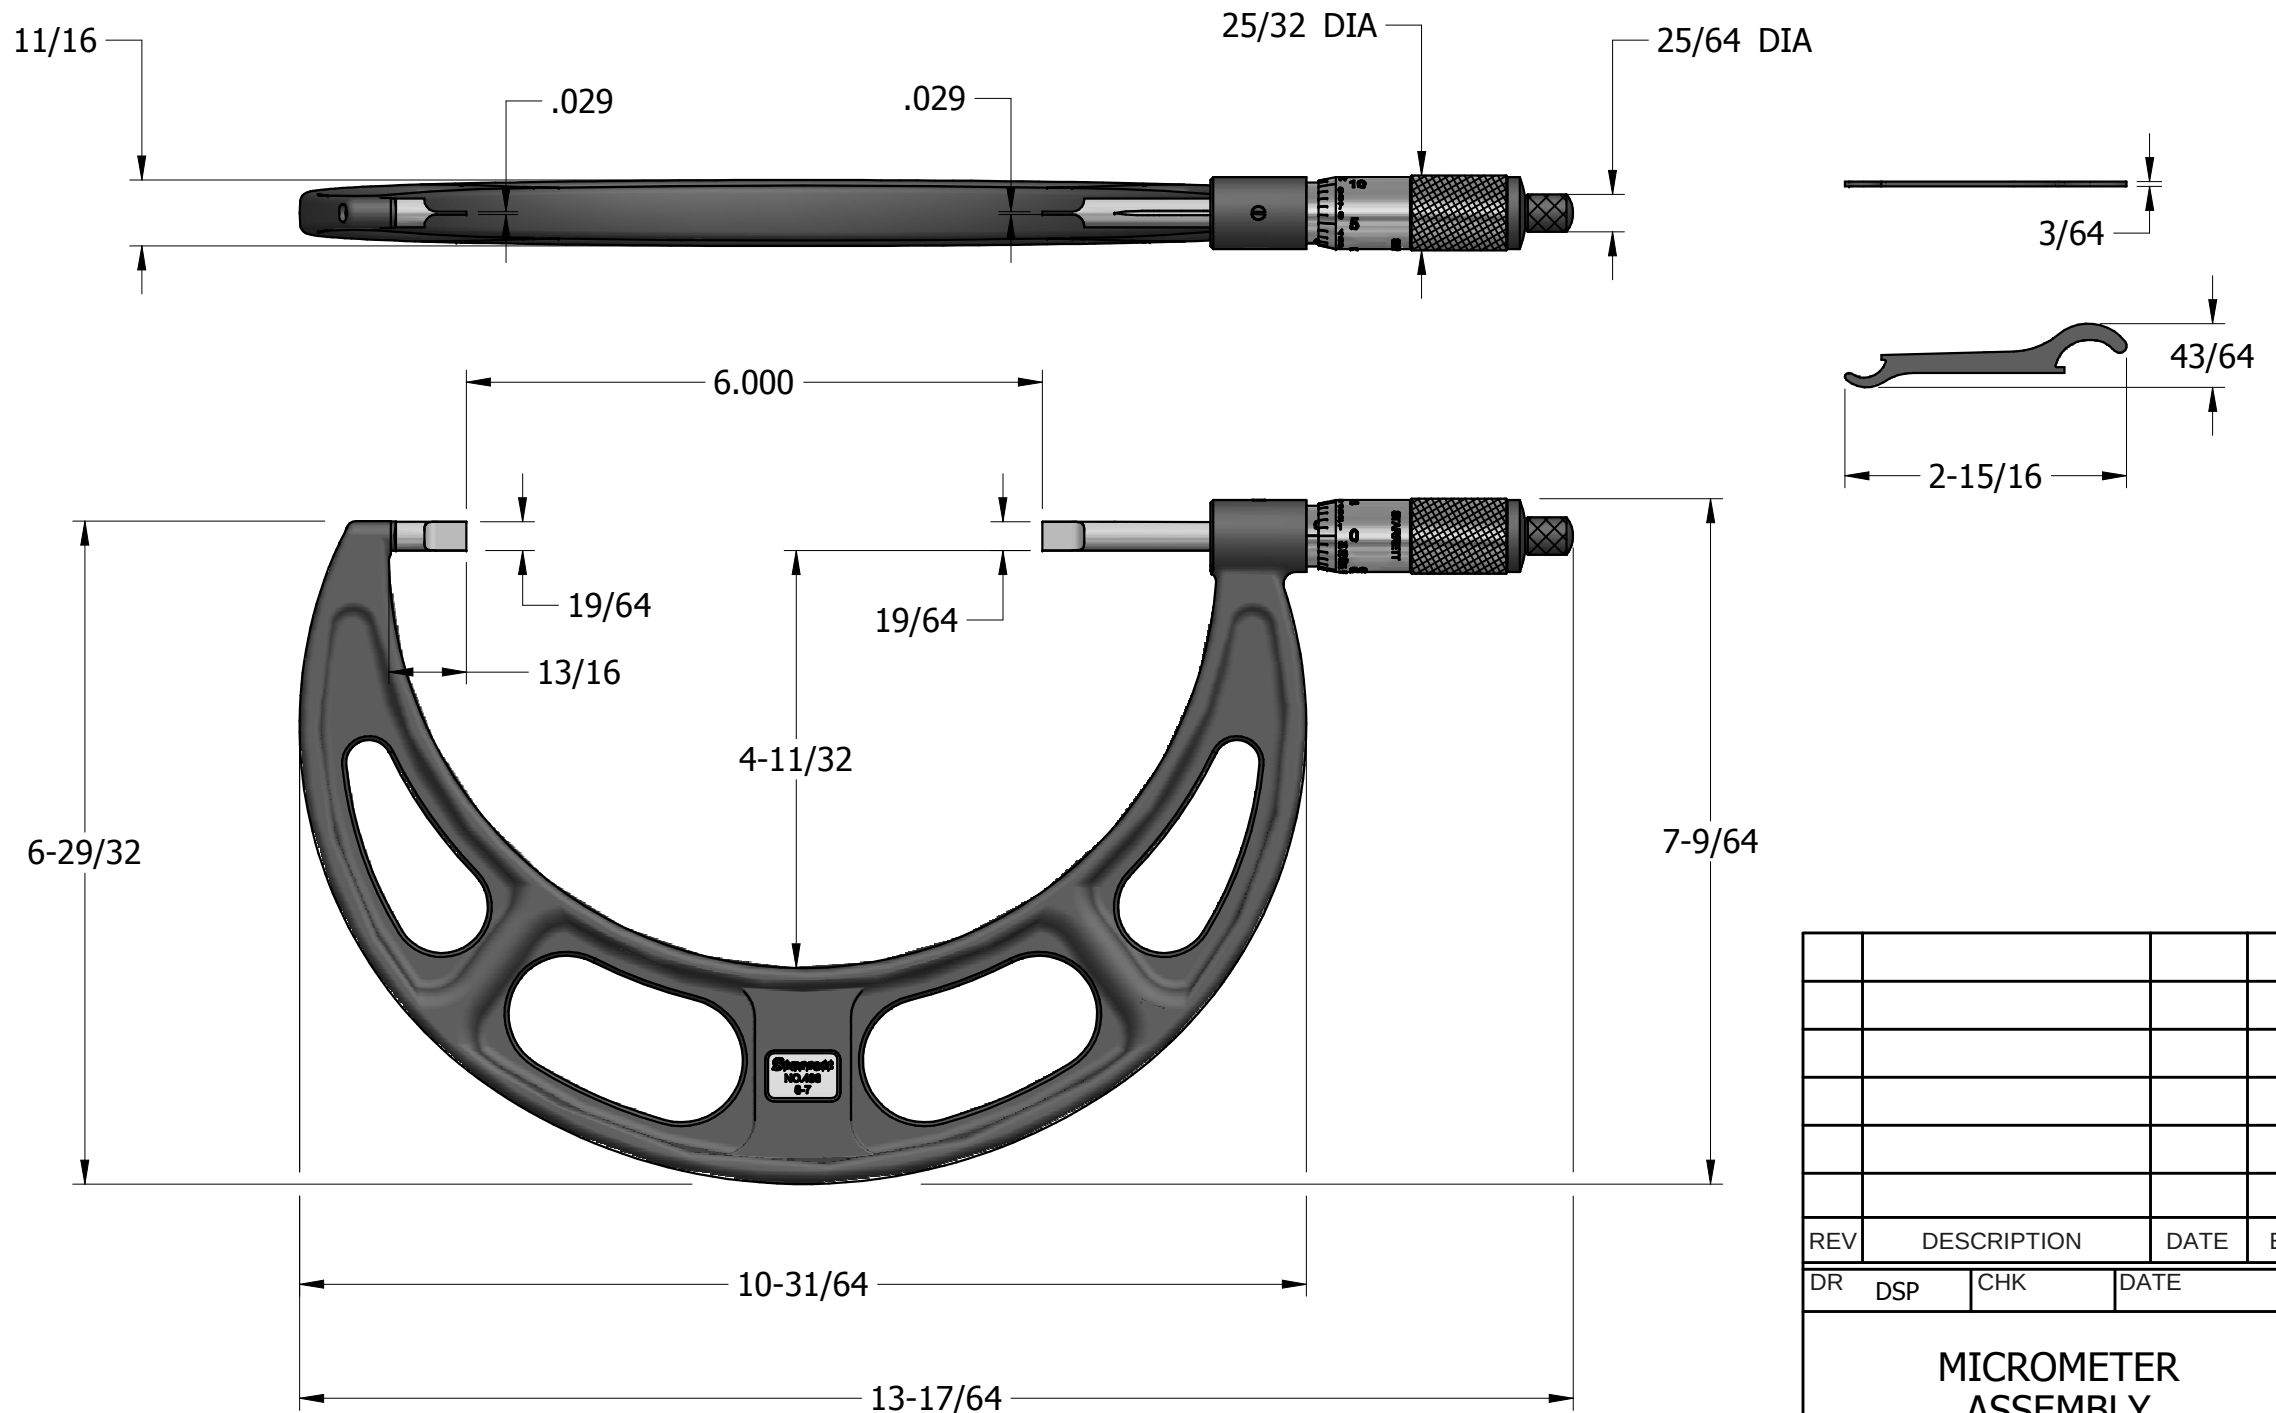

|                                       |             |      |      |
|---------------------------------------|-------------|------|------|
|                                       |             |      |      |
|                                       |             |      |      |
|                                       |             |      |      |
|                                       |             |      |      |
|                                       |             |      |      |
|                                       |             |      |      |
|                                       |             |      |      |
| REV                                   | DESCRIPTION | DATE | BY   |
| DR                                    | DSP         | CHK  | DATE |
| MICROMETER<br>ASSEMBLY                |             |      |      |
| THE L.S. STARRETT CO.<br>ATHOL, MASS. |             |      |      |

FRACTIONAL TOLERANCE  $\pm 1/64$  UNLESS OTHERWISE NOTED