


OPER	TOOLS

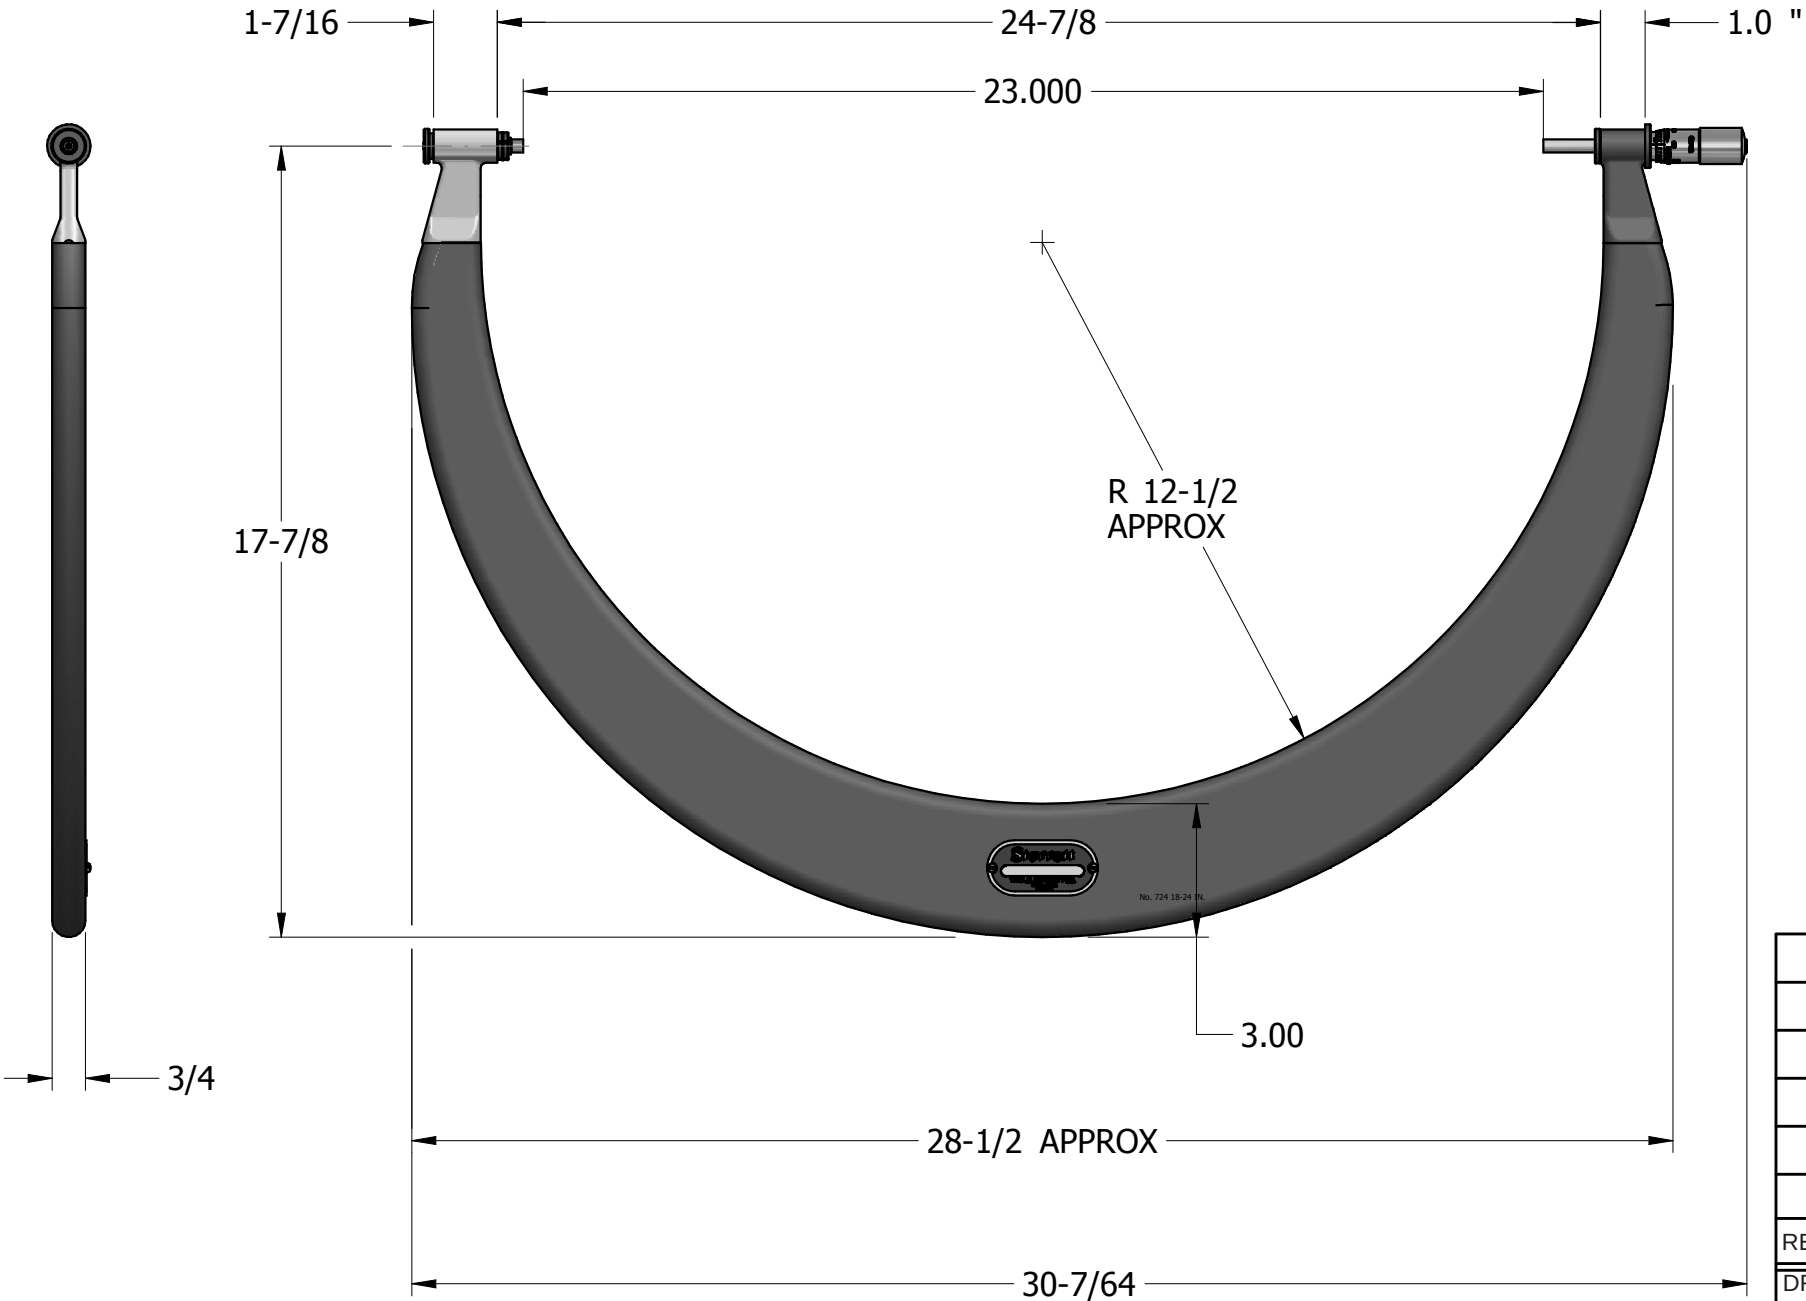

REV	DESCRIPTION	DATE	BY
-----	-------------	------	----

DR	CAP	CHK	DATE
----	-----	-----	------

TUBULAR BOW TYPE MICROMETER
W/INTERCHANGEABLE ANVILS
RANGE 18" - 24"

FRACTIONAL TOLERANCE $\pm 1/64$ UNLESS OTHERWISE NOTED

THE L.S. STARRETT CO.
ATHOL, MASS.