


OPER	TOOLS

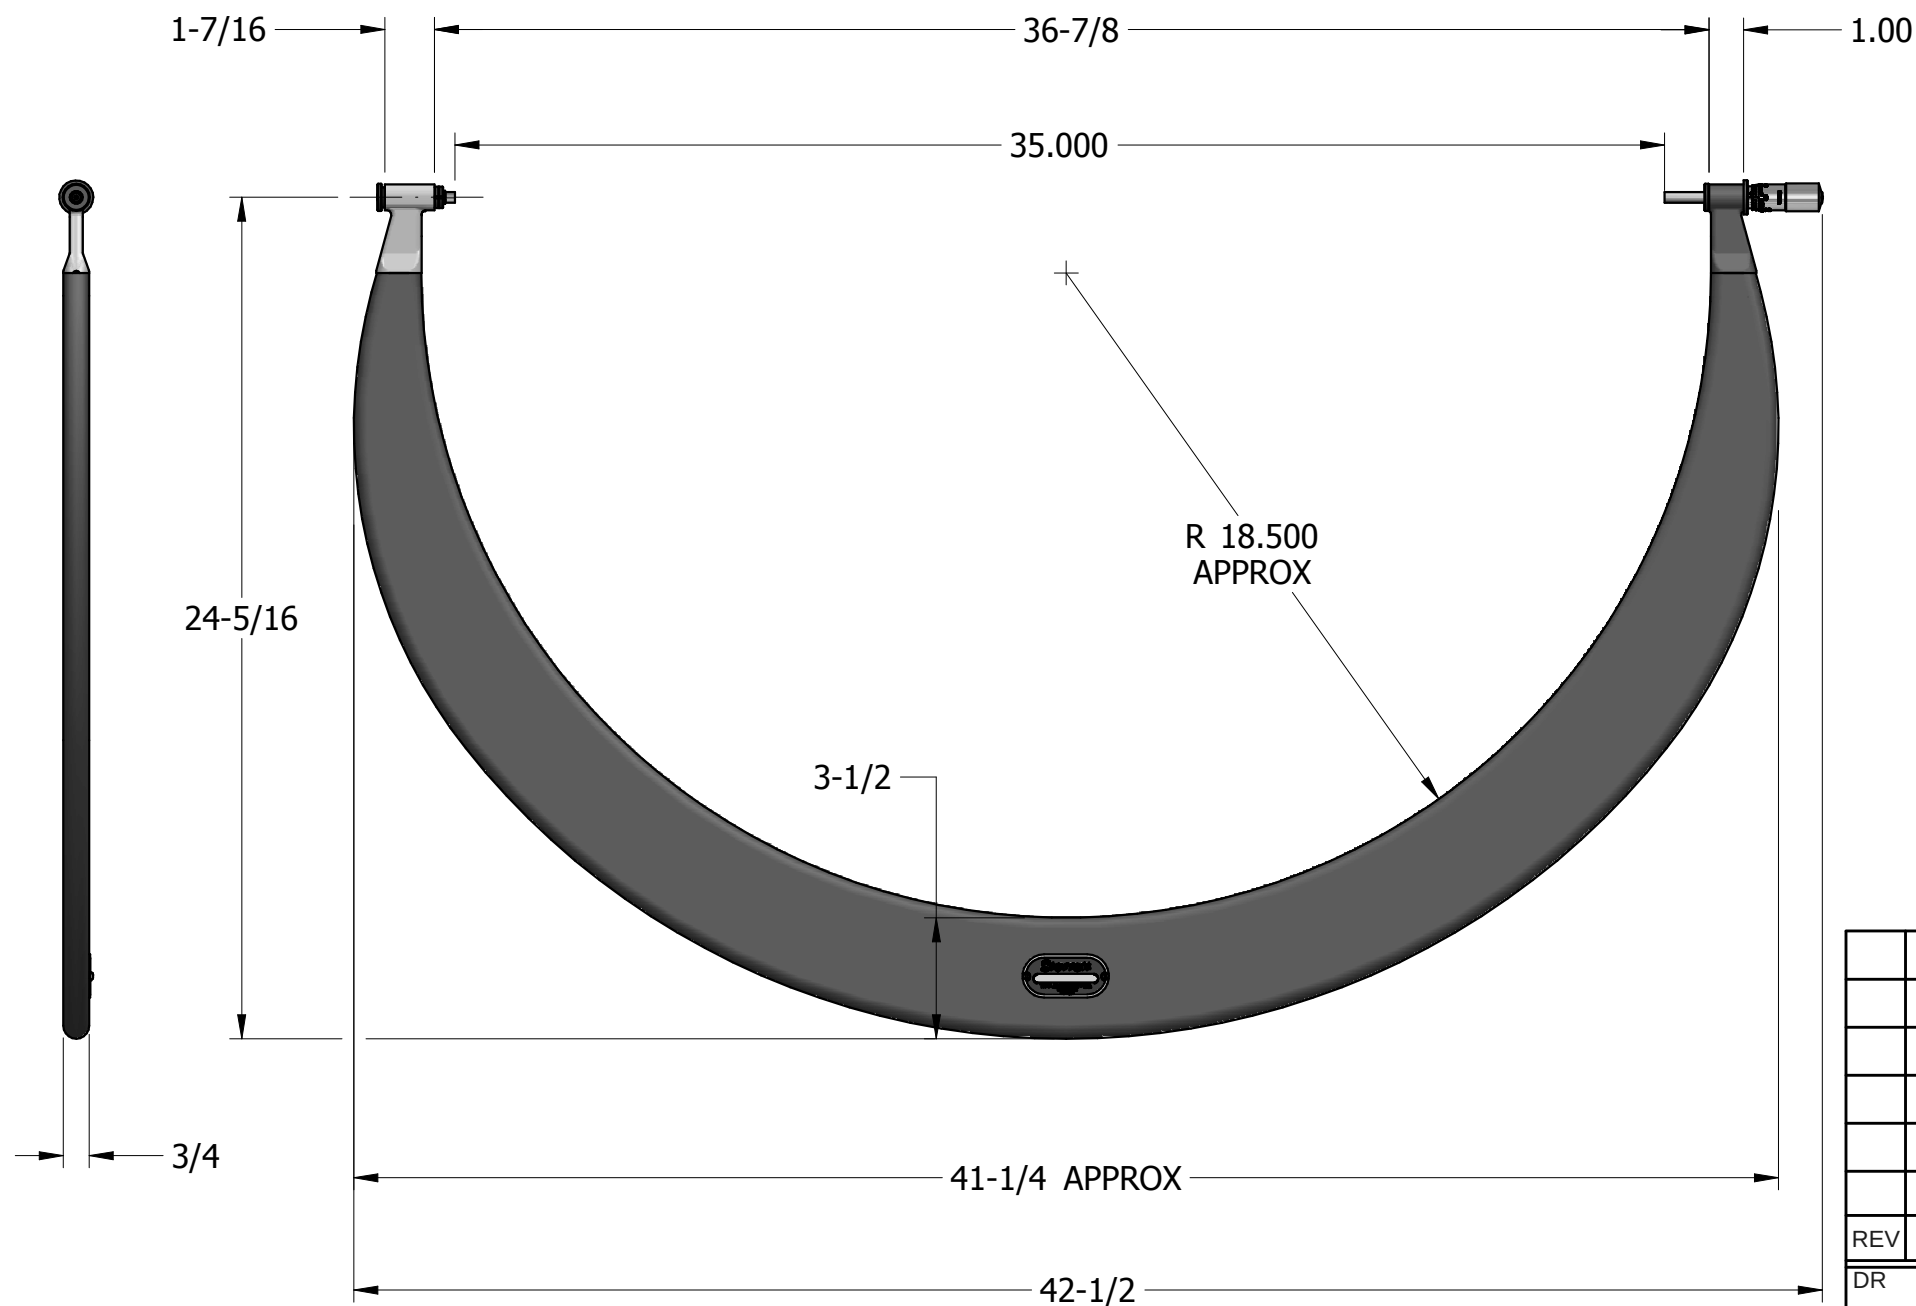

REV	DESCRIPTION	DATE	BY
DR	CAP	CHK	DATE
TUBULAR BOW TYPE MICROMETER W/INTERCHANGEABLE ANVILS RANGE 30" - 36"			
THE L.S. STARRETT CO. ATHOL, MASS.			

FRACTIONAL TOLERANCE $\pm \frac{1}{64}$ UNLESS OTHERWISE NOTED